


检验检测报告

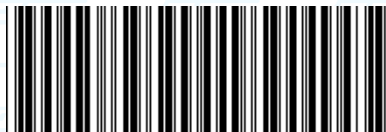

No:230016021

防伪查询网址: www.gttctech.com

防伪码: EEEB-4317-54

共3页 第1页

扫码下载报告



委托单位	广州市华滤环保设备有限公司 地址: 广州市番禺区沙头街大富村进村大街3号				
客户认定信息	滤材 50cm×50cm 颜色: 灰白 型号规格: 210*297 生产单位: 广州市华滤环保设备有限公司				
检验性质	委托检测	样品受理/测试开始日期	2023-01-09	报告签发日期	2023-02-02
判定依据	EN 1822-1:2019 《高效空气过滤器 (EPA, HEPA和ULPA) 第1部分: 分类、性能试验和标记》				
综合检验结论	---				
检验检测结果	检验检测项目	判定依据	判定		
	过滤性能	EN 1822-1:2019	符合		
备注	判定指标来源于客户要求的EN 1822-1:2019。我单位获CMA认定授权的检验能力覆盖EN 1822-1:2019所检项目。 本报告中检验检测项目均在相应标准规定的环境条件下进行 (有注明的除外)。 复印件、副本未重新加盖报告书确认章无效。 本报告检验检测地址为广州市番禺区珠江路1号。				

签发: 钟菊祥 工程师

钟菊祥



样品图片

No:230016021

共3页 第2页



检验检测报告附页

No: 230016021

共3页 第3页

过滤性能

测试方法: EN ISO 29463-3:2018, 单分散气溶胶计数法

气溶胶颗粒: NaCl


气体流量: 32L/min

试验面积: 100cm²
测试环境: 温度: 23.1℃, 相对湿度: 50.2%

测试结果:

粒径 (μm)	平均过滤效率 (%)	95%置信区间下限的平均过滤效率 (%)
0.015	99.82	99.81
0.03	98.9	98.9
0.06	96.9	96.9
0.1	97.3	97.3
0.15	98.3	98.3
0.2	99.03	99.03
0.3	99.58	99.56
平均压差 (Pa)	154.7	
最易穿透粒径MPPS (μm)	0.06	
最易穿透粒径MPPS对应的过滤效率 (%)	96.9	
技术要求	≥95% (E11) EN 1822-1:2019	
结论	符合	
备注	---	

平均过滤效率和粒径的关系曲线:

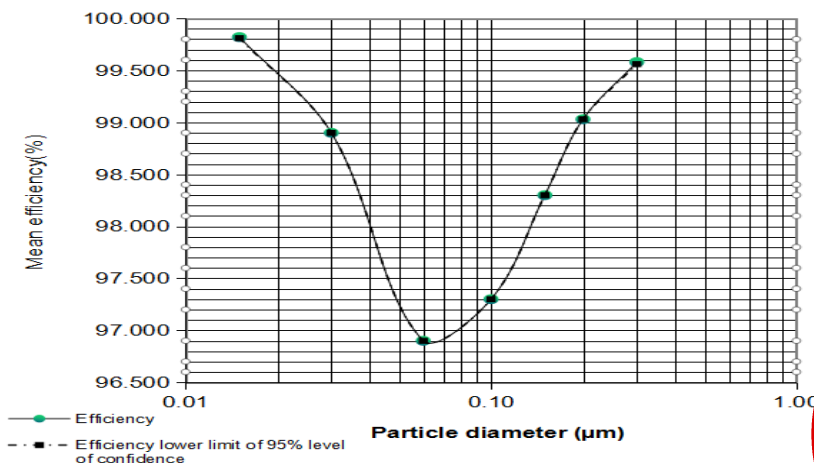

————本报告结束———



注意事项

1. 报告书未加盖检测单位检验检测专用章无效。
2. 复印件未加盖检测单位报告确认章无效。
3. 对委托送检结果有异议的，应于报告书送达之日起十五日内提出。
4. 检测结果仅对所检样品有效。
5. 未取得资质认定的项目，仅作为科研、教学或内部质量控制之用。
6. 报告书涂改无效。
7. 客户提供的信息（包括样品信息），本公司/中心不对其真实性负责。
8. 未经本公司/中心书面批准不得部分复制本报告，全部复制除外。

Note

1. The report is invalid without authorized stamp.
2. Copies of this report are invalid without authorized stamp.
3. Any dispute should be raised within 15 days after receiving the report.
4. The result is only valid for the tested sample.
5. The results of unapproved items are for reference only.
6. This report is invalid if altered.
7. Our company does not accept any responsibility for the authenticity of the information supplied by customers (including sample information).
8. The report shall not be duplicated separately or partly, without prior written permission approved by GTTC, except duplicated in full version.